

---

## Station Information Report

# Solar and Meteorological Station

Pacific Power Association - Nauru

---



| Revision | Date         | Author         | Checked           | Approved    | Comments    |
|----------|--------------|----------------|-------------------|-------------|-------------|
| Rev 0    | 1 April 2020 | M.D. Johnstone | J. van Jaarsveldt | M. de Jager | First Issue |
| Rev 1    |              |                |                   |             |             |
| Rev 2    |              |                |                   |             |             |

## Contents

|    |  |    |
|----|--|----|
| 1  | Introduction .....                                     | 2  |
| 2  | Station Summary .....                                  | 3  |
| 3  | Map of area.....                                       | 4  |
| 4  | Site layout.....                                       | 5  |
| 5  | Instrument list, serial numbers and multipliers.....   | 7  |
| 6  | Supporting hardware and communication peripherals..... | 8  |
| 7  | Data logger wiring .....                               | 8  |
| 8  | Power circuit diagram.....                             | 10 |
| 9  | Detail Photographs .....                               | 11 |
| 10 | Terrain Photographs.....                               | 18 |
| 11 | Station Photographs.....                               | 25 |
| 12 | Calibration Certificates .....                         | 32 |

## 1 Introduction

The World Bank initiated the Sustainable Energy Industry Development Project (SEIDP) to, amongst others, support the Pacific Power Association (PPA) in doing renewable energy resource assessments. The focus for this particular section of the project is to get high quality bankable wind as well as irradiance measurements supported by high quality meteorological measurements and to promote the awareness of the resource potential of wind and solar energy.

GeoSUN Africa is to execute the on-site measurement related aspects of the solar section of the project. The assignment for GeoSUN Africa is the following:


- An inception mission which involves visiting the proposed site locations and selecting the optimal location for the measurement equipment. The outcome of this inception mission is this implementation plan where sites and stations tiers are proposed;
- Providing high quality measuring equipment for each site, in line with the technical specifications;
- Installation of measurement equipment as well as subsequent Site Installation Report and photographs for each site;
- Hosting and providing two years of high quality, 'bankable' meteorological data relevant for solar resource assessment and project development;
- Ensuring maintenance, security, local cleaning/caretaking, and mitigation against extreme weather events and corrosion;
- Ensuring strong local involvement and capacity building at all stages of the measurement campaign;
- Decommissioning of all sites at the end of the measurement campaign, unless separate arrangements are made with one or more host institutions to continue with measurements outside of this assignment/contract.

This document acts as the Site Installation Report which follows the commissioning of the site, outlining the site location, site characteristics, technical specifications, calibration procedures, and all other relevant information to allow data users to fully understand the site and ensure the bankability of the measurement data. The Site Installation Report contains photographs of the site and the surrounding terrain.

The measurement data from the site will be continuously transferred to GeoSUN's central data repository, and shall then be transferred to the PPA on a monthly basis in both raw and quality-controlled formats according to the specifications developed by ESMAP. This data will be delivered via an online file sharing platform one month in arrears. Site Measurement Reports will accompany the delivery of monthly data, and shall detail any issues with the site or equipment, field calibration procedure, and any notable conclusions or results.

The assignment shall be deemed completed once two years of concurrent data is delivered in compliance with the minimum data recovery rates specified. At this point the vendor shall decommission each site and remove the solar measurement equipment, unless alternative arrangements outside the scope of this assignment/contract are made and endorsed by the relevant client/host agency.

## 2 Station Summary
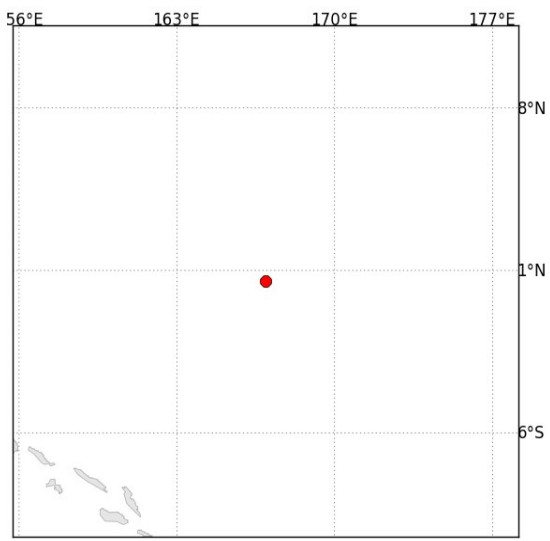
|  |  |
|--|--|
| <b>Work performed</b>  | Installation and commissioning of solar and meteorological measurement station   |
| <b>Commissioning date</b>                                    | 25 January 2020  |
| <b>Planned decommissioning date</b>                          | 25 January 2022  |
| <b>Client</b>  | Pacific Power Association  |
| <b>Client contact person and contact details</b>             | Name: Wairarapa J. Young<br>Email: rapa@ppa.org.fj<br>Telephone: (679) 330 6022  |
| <b>Site location</b>   | <p>Nauru Utilities Corporation Meneng PV Power Plant.</p>   |
| <b>Access</b>  | From Meneng Hotel, take the Island ring road until you reach a dirt road heading towards the centre of the Island. Follow the road to a Y-intersection and take a sharp left. Continue for around 1.5 km and the solar plant will be on your left. |
| <b>Coordinates</b>   | 0°32'36.4"S 166°55'55.1"E<br>(-0.543447, 166.931970)   |
| <b>Elevation</b>   | 28 m AMSL  |
| <b>Time zone (local and data logger)</b>                     | GMT +12 local time zone  |
| <b>Name and contact details of on-site contact person(s)</b> | Name: Apenisa Manuduitagi<br>Phone: (674) 557 4069   |



### 3 Map of area

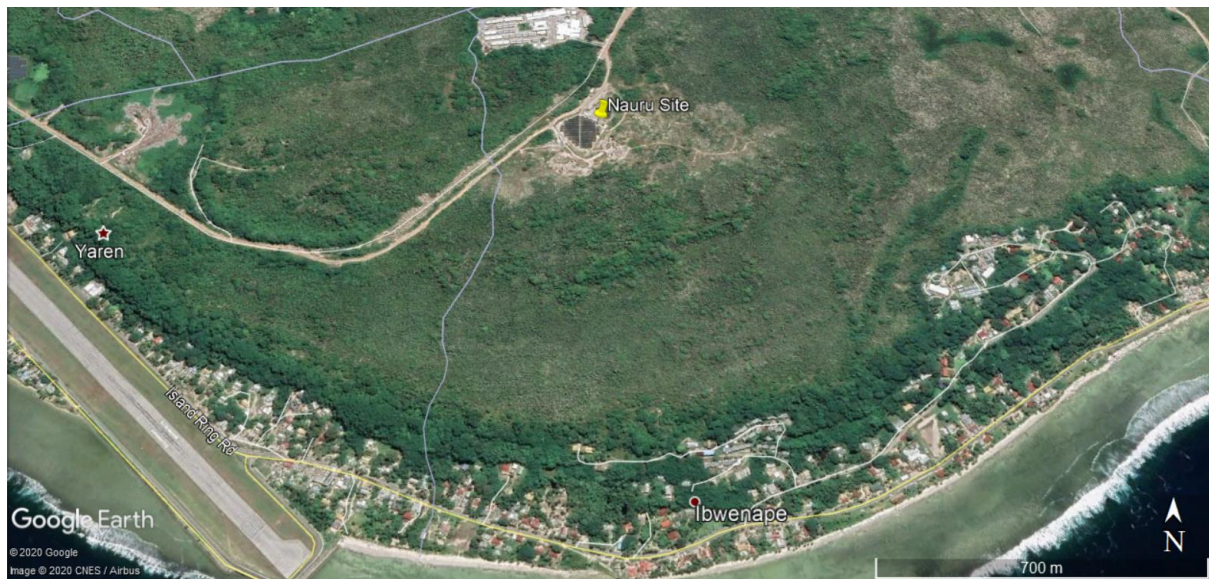


Figure 1: Map of the surrounding area (Source: Google Earth)

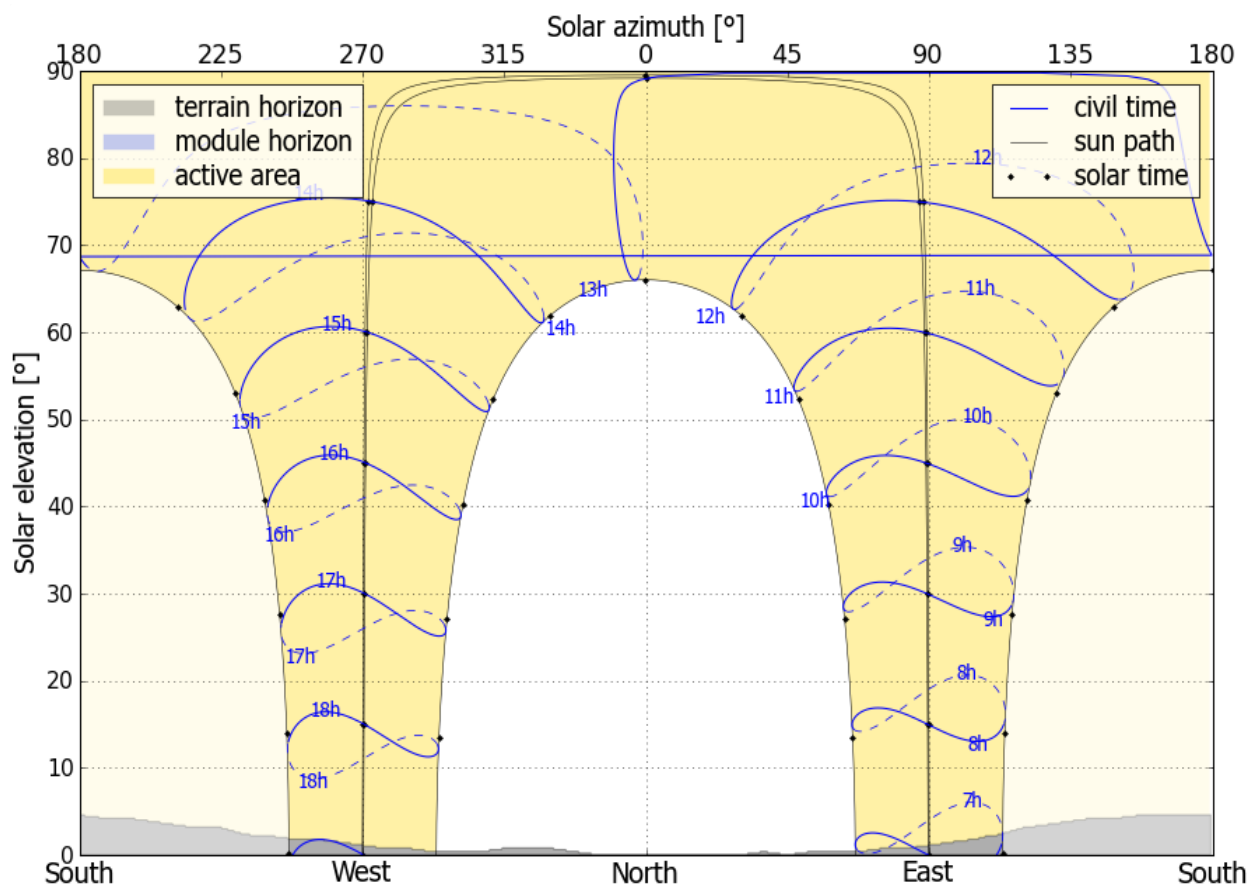


Figure 2: Terrain horizon and day length (Source: Solargis)

## 4 Site layout

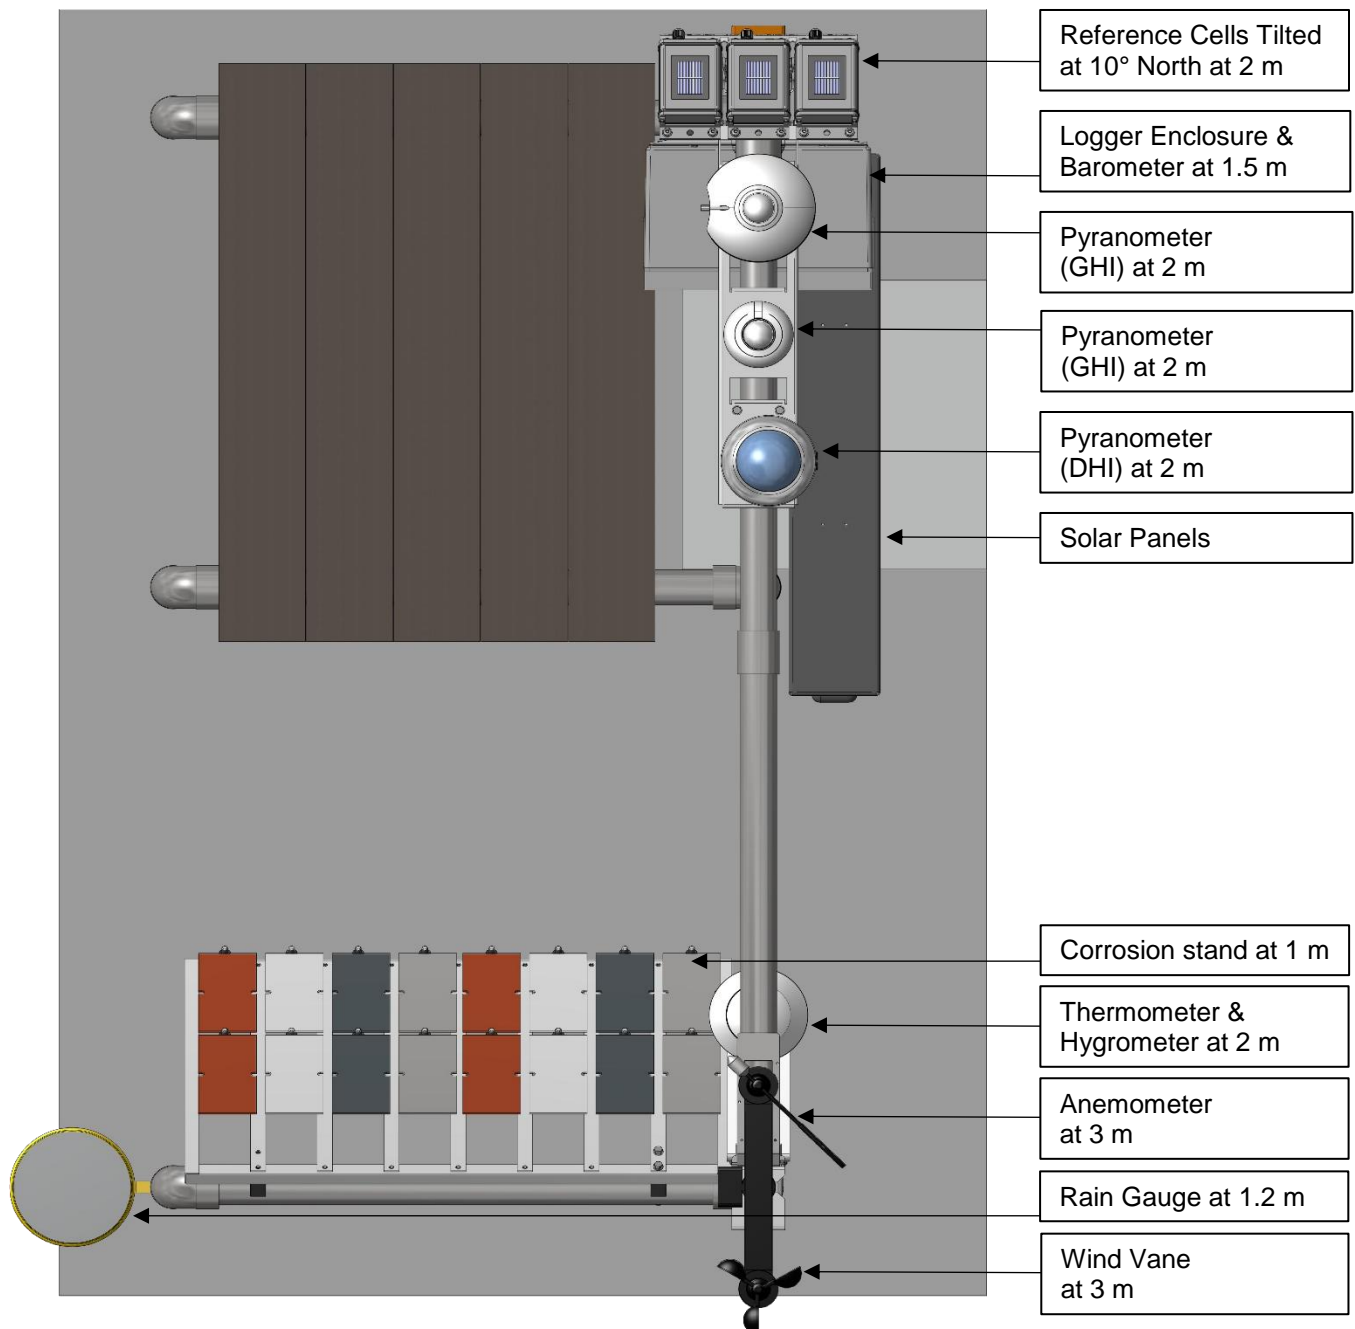


Figure 3: Site Layout (plan view)

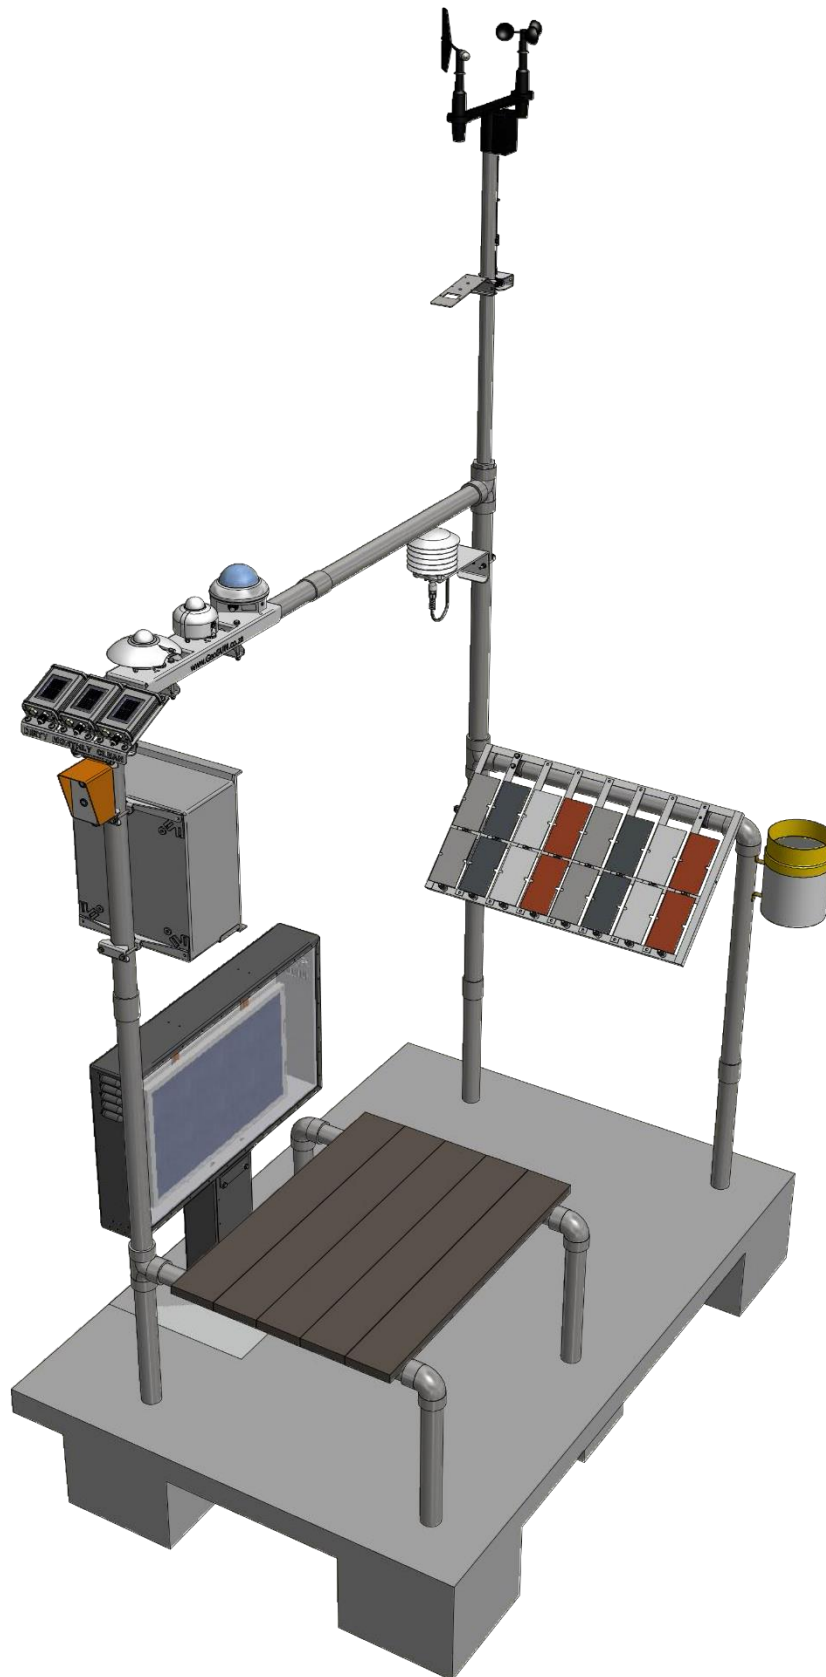


Figure 4: Site Layout (perspective view)

## 5 Instrument list, serial numbers and multipliers

| Instrument (Measurement)                         | Make and Model                 | Serial Number        | Variable Name (Program) | Multiplier                |
|--|--------------------------------|----------------------|-------------------------|---------------------------|
| Pyranometer (GHI)                                | Hukseflux SR30-D1              | 4271                 | GHI_1                   | 10.41 $\mu\text{V/W/m}^2$ |
| Pyranometer (GHI)                                | Hukseflux SR20-T2              | 10546                | GHI_2                   | 15.87 $\mu\text{V/W/m}^2$ |
| Pyranometer (DHI)                                | Delta Electronics SPN 1        | A2057                | GHI_SPN1                | 1                         |
| Reference Cell Clean                             | Ingenieurbüro Si-mV-85-A       | 85-00205-17-19350068 | RefCellClean            | 58.25 $\mu\text{V/W/m}^2$ |
| Reference Cell Monthly                           | Ingenieurbüro Si-mV-85-A       | 85-00205-17-19350069 | RefCellMonthly          | 57.62 $\mu\text{V/W/m}^2$ |
| Reference Cell Dirty                             | Ingenieurbüro Si-mV-85-A       | 85-00205-17-19350076 | RefCellDirty            | 57.93 $\mu\text{V/W/m}^2$ |
| 3-Cup Anemometer (Wind speed)                    | RM Young 03002                 | 016673               | WSpd                    | 0.2 Offset<br>0.75 Slope  |
| Wind Vane (Wind Direction)                       | RM Young 03002                 | 016673               | WDir                    | 0 Offset<br>352 Slope     |
| Temperature Sensor (Ambient Temperature)         | Campbell Scientific CS215      | E22431               | Temp                    | 1                         |
| Relative humidity Sensor (Relative Humidity)     | Campbell Scientific CS215      | E22431               | RH                      | 1                         |
| Barometer (Atmospheric Pressure)                 | Vaisala PTB110                 | R3331024             | BP                      | 500 offset<br>0.24 slope  |
| Rain Gauge (Rain)                                | Texas Electronics TR-525I      | 81181-819            | Rain                    | 0.2 mm/tip                |
| Corrosion Plate                                  | Make                           | Sample               | Position (Column, Row)  | Mass (g)                  |
| Mild Steel plate (Corrosion Testing)             | Orytech Mild Steel             | E1                   | C2,R1                   | 133.3570                  |
|  |                                | E2                   | C2,R2                   | 131.5444                  |
|  |                                | E3                   | C6,R1                   | 133.6663                  |
|  |                                | E4                   | C6,R2                   | 137.4902                  |
| H.D. Galvanised (Zinc) plate (Corrosion Testing) | Orytech H.D. Galvanised (Zinc) | E1                   | C3,R1                   | 82.1905                   |
|  |                                | E2                   | C3,R2                   | 83.2209                   |
|  |                                | E3                   | C7,R1                   | 80.4325                   |
|  |                                | E4                   | C7,R2                   | 82.2611                   |
| Copper plate (Corrosion Testing)                 | Orytech Copper                 | E1                   | C1,R1                   | 81.3126                   |
|  |                                | E2                   | C1,R2                   | 82.4692                   |
|  |                                | E3                   | C5,R1                   | 81.5095                   |
|  |                                | E4                   | C5,R2                   | 83.7698                   |
| Aluminium plate (Corrosion Testing)              | Orytech Aluminium              | E1                   | C4,R1                   | 38.2537                   |
|  |                                | E2                   | C4,R2                   | 37.4995                   |
|  |                                | E3                   | C8,R1                   | 37.2818                   |
|  |                                | E4                   | C8,R2                   | 37.6965                   |

## 6 Supporting hardware and communication peripherals

|                     |   |
|---------------------|---|
| Data Logger         | Campbell Scientific CR1000X (OS: Std.03.02)                     |
| Communication       | RS232 (115200) TCP/IP   |
| Pakbus Address      | 783   |
| Password Set        | None  |
| Modem               | Maestro M100 3G modem with Poynting antenna                     |
| Network Details     | Service provider: Digitcel, Nauru<br>Phone number: 674 554 1483 |
| Modem Power Control | SW12V   |
| Data Logger Clock   | GMT+12  |
| Main Battery        | 2 x 12 V / 24 Ah  |
| Solar Panel(s)      | 2 x 25 W  |
| Charge Controller   | 2 x CPL Research (10 A)   |

## 7 Data logger wiring

| PPA Wiring Diagram<br>November 2019- CR1000x |                    |            |                          |          |          |            |      |
|--|--------------------|------------|--------------------------|----------|----------|------------|------|
|  |                    |            |                          |          |          |            |      |
| Logger Port                                  | Accessories        | Connection | Instrument Cable         | Function | Reading  | Instrument |      |
|  | 250mA Fast-Blow    | C7         | Grey                     | A-       | GHI1     | SR30       |      |
|  |                    | C8         | White                    | B+       |          |            |      |
|  |                    | AGB        | Shield                   | GND      |          |            |      |
|  |                    | PB-Fused   | Brown                    | 12V      |          |            |      |
|  |                    | GB         | Black                    | 0V       |          |            |      |
|  |                    |            | Blue                     | NC       |          |            |      |
|  |                    |            | 3H                       | White    | Signal + | GHI2       | SR20 |
|  |                    |            | 3L                       | Green    | Signal - |            |      |
|  |                    |            | AGB                      | Black    | GND      |            |      |
|  | SW12-2             |            | Yellow                   | Heater + |          |            |      |
|  | G                  | Brown      | Heater -                 |          |          |            |      |
| VX1  | 10kΩ 0.1% Resistor | SE4        | Red+Pink                 | Temp +   |          |            |      |
|  |                    | AG2        | Blue+Grey                | Temp -   | DHI      | SPN1       |      |
|  |                    | 5H         | White                    | GHI +    |          |            |      |
|  |                    | 6H         | Brown                    | DHI +    |          |            |      |
|  |                    | 5L         | Green                    | Signal - |          |            |      |
|  |                    | 6L         | Bridged with 5L/Signal - |          |          |            |      |
|  |                    | GB         | Grey                     | 0 V      |          |            |      |
|  |                    | PB         | Pink                     | 12 V     |          |            |      |

|        |      |              |            |                        |                |
|--------|------|--------------|------------|------------------------|----------------|
| SW12-2 |      | Red          | Heater +   |                        |                |
|        | G    | Blue         | Heater -   |                        |                |
|        | AGB  | Clear        | GND        |                        |                |
|        | NC   | Yellow       | Sun        |                        |                |
|        | PB   | Red          | 12 V       | Temp & RH              | CS215          |
|        | C1   | Green        | Signal +   |                        |                |
|        | GB   | White        | 0 V        |                        |                |
|        | GB   | Black        | 0 V        |                        |                |
|        | AGB  | Clear        | GND        | Clean                  | Ref cell       |
|        | SE13 | Orange       | Signal +   |                        |                |
|        | AG6  | Blue         | Signal -   |                        |                |
|        | AGB  | Black        | GND        | Monthly                | Ref cell       |
|        | SE14 | Orange       | Signal +   |                        |                |
|        | AG7  | Blue         | Signal -   |                        |                |
|        | AGB  | Black        | GND        | Dirty                  | Ref cell       |
|        | SE15 | Orange       | Signal +   |                        |                |
|        | AG7  | Blue         | Signal -   |                        |                |
|        | AGB  | Black        | GND        | Wind Speed & Direction | 03002          |
|        | VX2  | Blue         | Excitation |                        |                |
|        | SE16 | Green        | Signal +   |                        |                |
|        | AG8  | White        | Signal -   |                        |                |
|        | AGB  | Clear        | GND        |                        |                |
|        | P1   | Red          | Signal +   | Rain                   | TE525          |
|        | AGB  | Clear        | GND        |                        |                |
|        | P2   | Black        | Signal +   |                        |                |
|        | AG   | White        | Signal -   | Clean                  | Clean Button   |
|        | AGB  | Clear        | GND        |                        |                |
|        | C5   | Red          | Signal +   |                        |                |
|        | C2   | Green        | Light +    |                        |                |
|        | C3   | Blue         | Signal -   | Monthly                | Monthly Button |
|        | AGB  | Clear        | GND        |                        |                |
|        | C4   | Yellow       | Signal +   |                        |                |
|        | C2   | Green        | Light +    |                        |                |
|        | C3   | Blue         | Signal -   | Gate                   | Switch         |
|        | AGB  | Clear        | GND        |                        |                |
|        | C6   | Red          | Signal +   |                        |                |
|        | G    | Blue         | Signal -   | Pressure               | PTB110         |
|        | AGB  | Clear        | GND        |                        |                |
|        | SE7  | Blue/Brown   | Signal +   |                        |                |
|        | 12V  | Red          | 12V        |                        |                |
|        | 5V   | Green        | Signal +   |                        |                |
|        | G    | Black        | Signal -   |                        |                |
|        | AG   | Yellow/White | GND        |                        |                |
|        | AG   | Clear        | GND        |                        |                |

## 8 Power circuit diagram

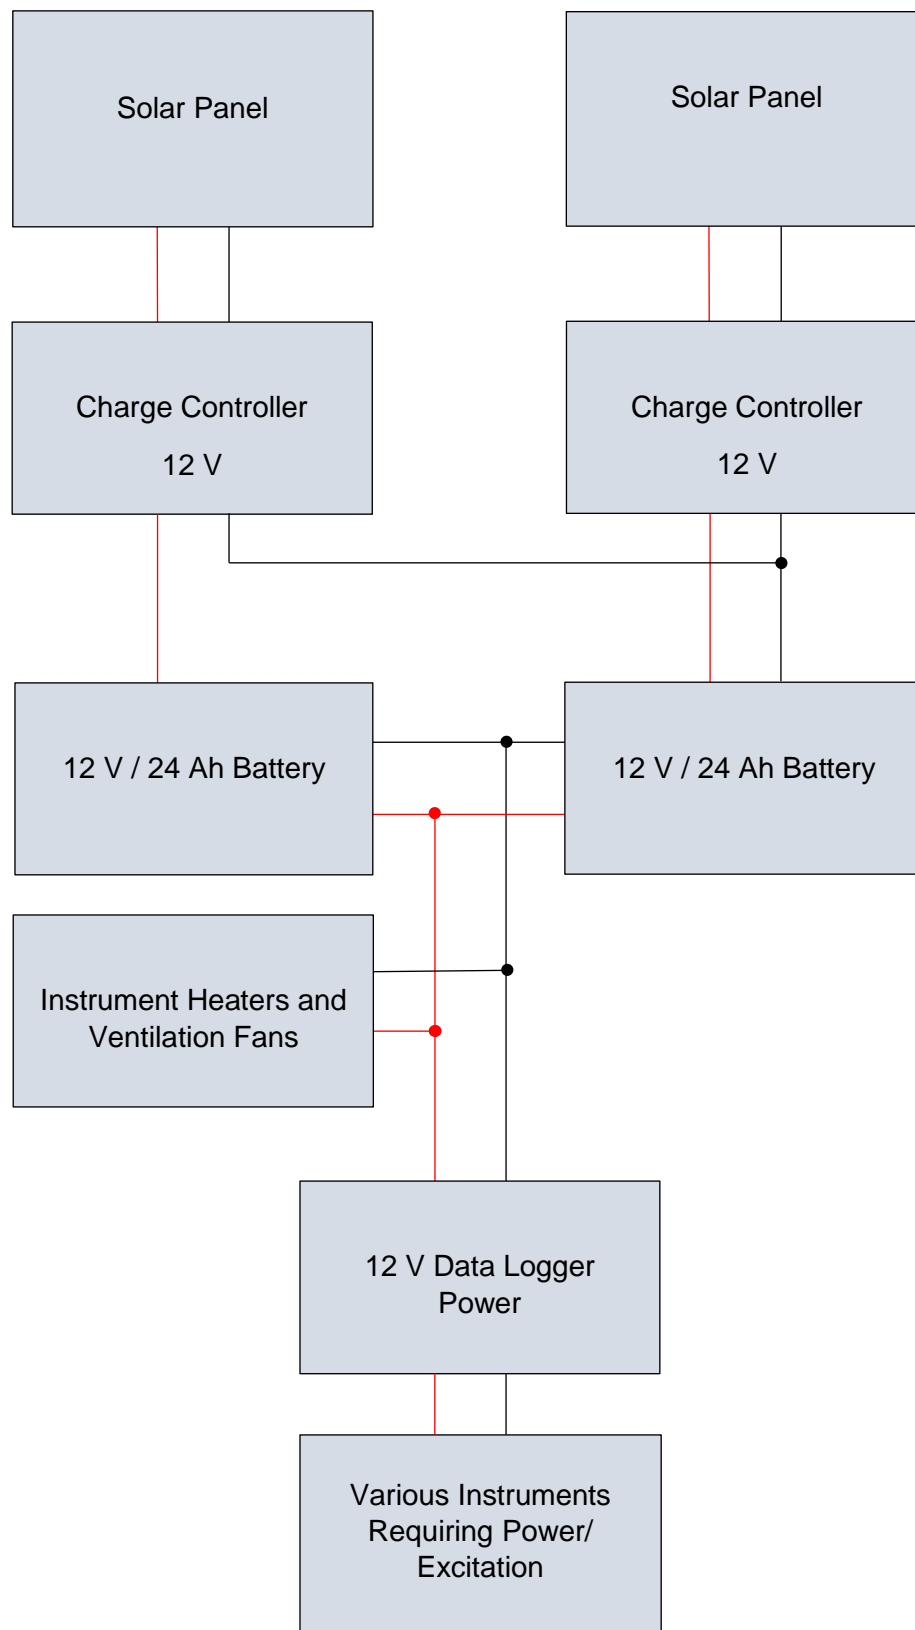


Figure 5: The DC power circuit



## 9 Detail Photographs

This section showcases details of the installation, including the main station components. Records are shown of instrument makes, models and serial numbers, as well as the installation levels and orientation where applicable.

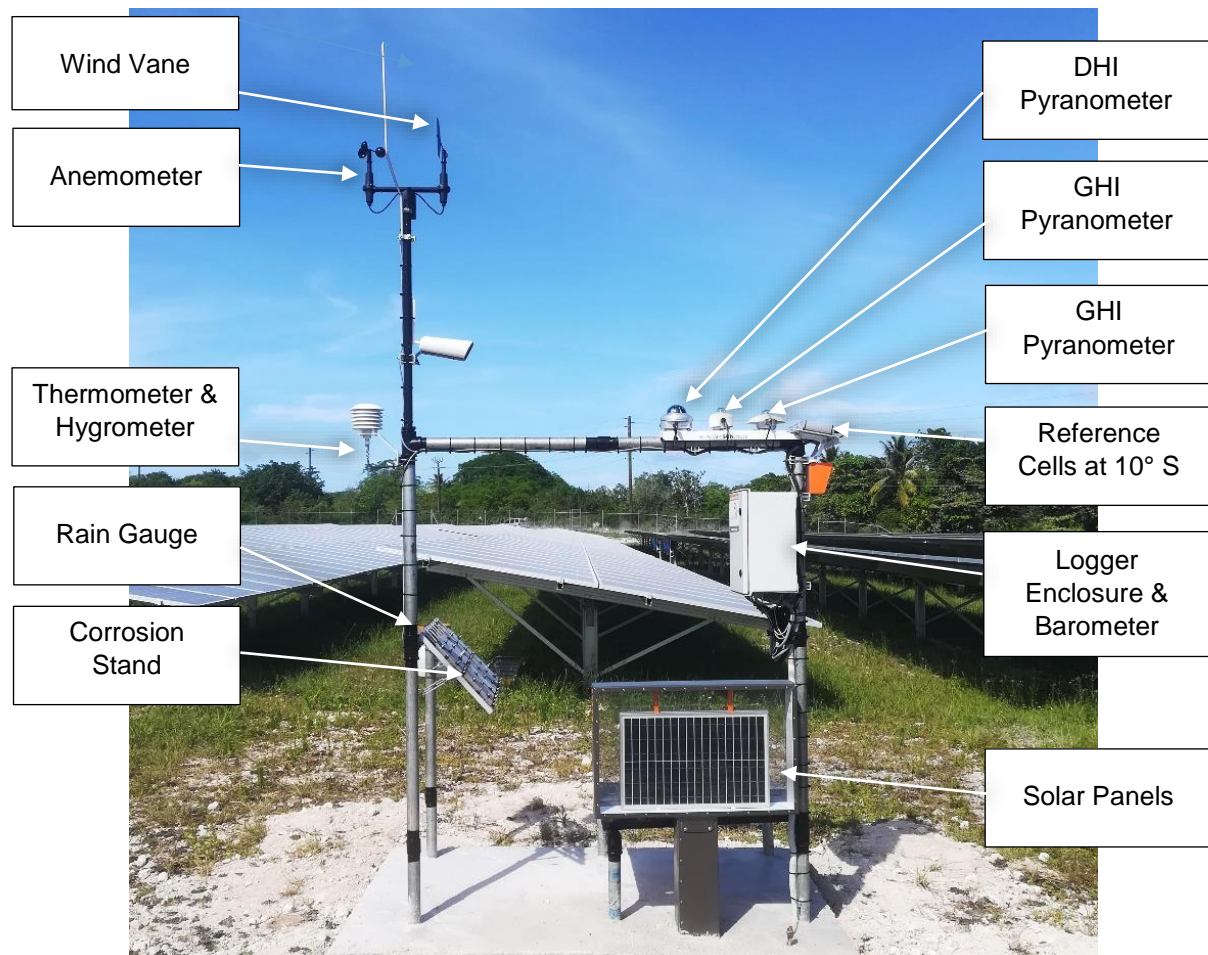


Figure 6: Station Summary

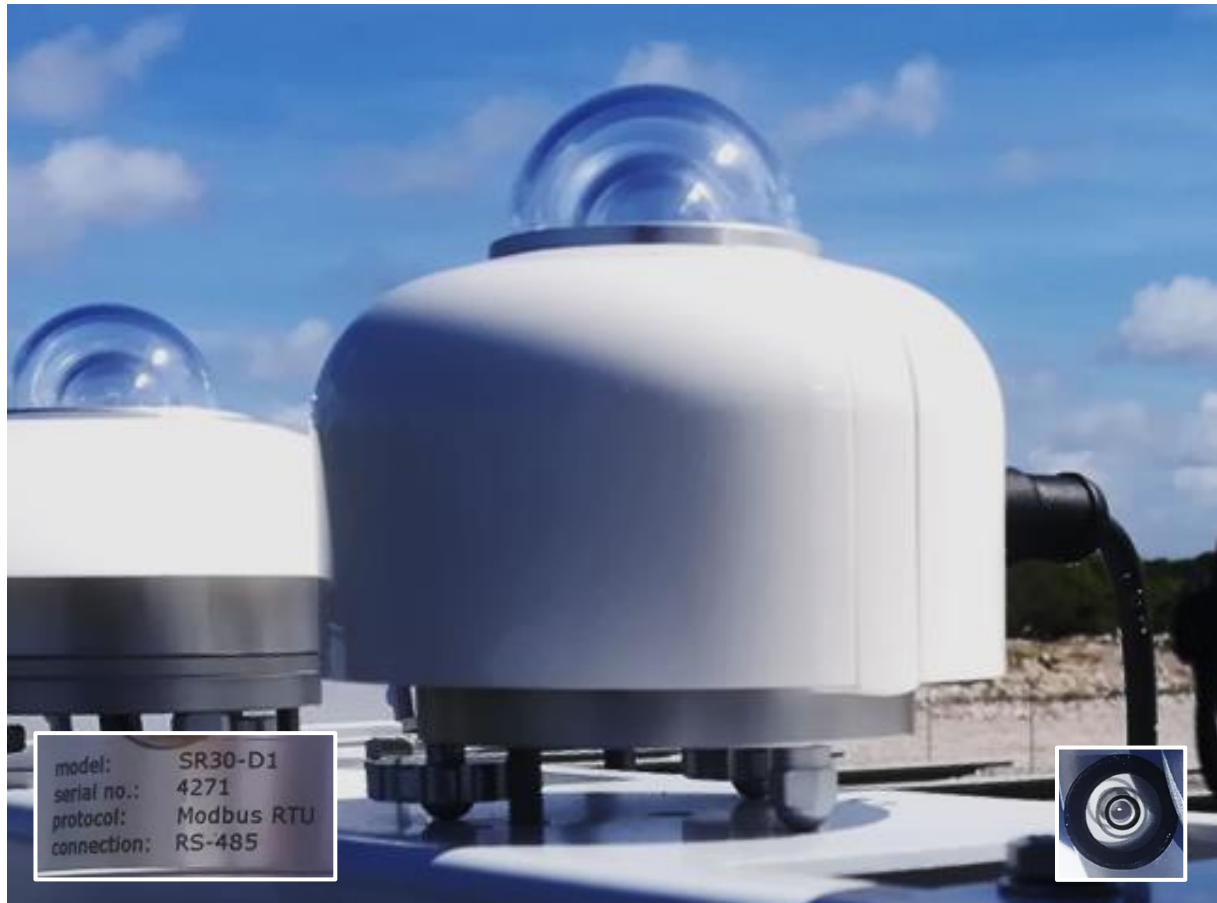


Figure 7: GHI (1) Pyranometer Installation



Figure 8: GHI (2) Pyranometer Installation



Figure 9: DHI Pyranometer Installation



Figure 10: Wind instruments at 3 m





Figure 11: Thermometer and Hygrometer at 2 m



Figure 12: Corrosion Test Stand



Figure 13: Rain Gauge

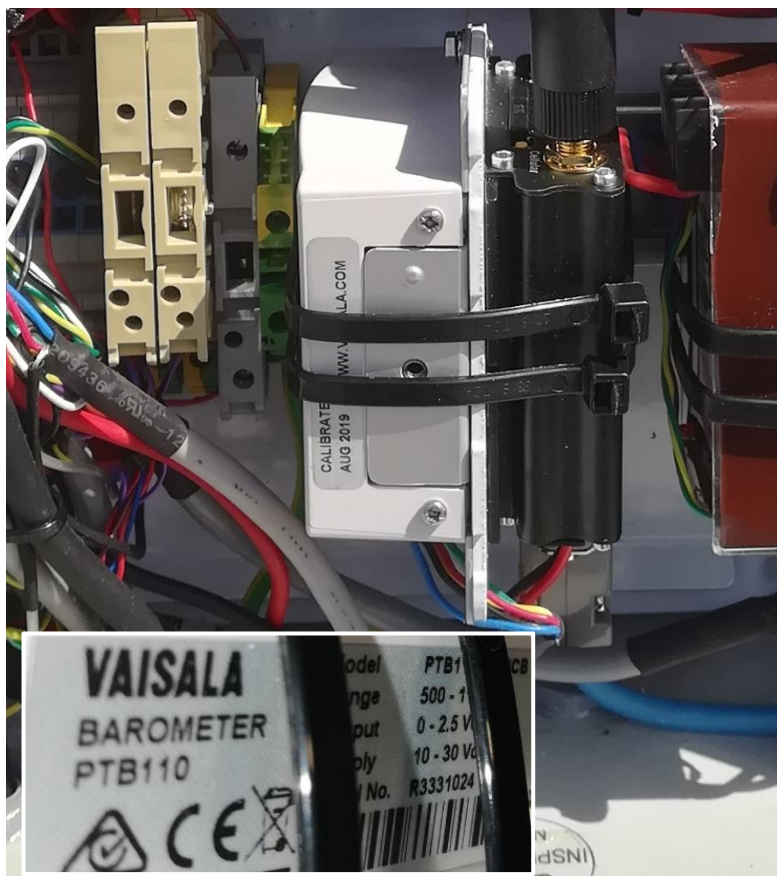


Figure 14: Barometer





Figure 15: Reference Cells at 10° North



Figure 16: Solar Panel



Figure 17: Logger Enclosure



## 10 Terrain Photographs

Obstacles protruding higher than the horizon as viewed from the solar instruments will affect lower solar elevation readings if they fall within the sun path as depicted in Figure 2. The pictures in this section shows the terrain surrounding the station at the time of installation, giving an indication of near or far shading influences on the station.



Figure 18: 0/360 Degrees (North)



Figure 19: 30 Degrees



Figure 20: 60 Degrees





Figure 21: 90 Degrees (East)



Figure 22: 120 Degrees



Figure 23: 150 Degrees



Figure 24: 180 Degrees (South)





Figure 25: 210 Degrees



Figure 26: 240 Degrees



Figure 27: 270 Degrees (West)



Figure 28: 300 Degrees





Figure 29: 330 Degrees



## 11 Station Photographs

This section indicates the station within the surrounding terrain to give an overall view thereof, as well as provide additional context to the possible near and far shading influences.



Figure 30: 0/360 Degrees (From North)



Figure 31: 30 Degrees



Figure 32: 60 Degrees





Figure 33: 90 Degrees (From East)



Figure 34: 120 Degrees





Figure 35: 150 Degrees



Figure 36: 180 Degrees (From South)





Figure 37: 210 Degrees



Figure 38: 240 Degrees





Figure 39: 270 Degrees (From West)



Figure 40: 300 Degrees



Figure 41: 330 Degrees



## 12 Calibration Certificates



**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

### Calibration certificate

Pages 1  
Release date: 24 SEP, 2019

Product code **SR30-D1**  
Product identification **serial number 4271**  
Product type pyranometer  
Measurand hemispherical solar radiation

#### Calibration result

Sensitivity  $S = 10.41 \times 10^{-6} \text{ V/(W/m}^2\text{)}$   
Calibration uncertainty  $\pm 0.10 \times 10^{-6} \text{ V/(W/m}^2\text{)}$

the number following the  $\pm$  symbol is the expanded uncertainty with a coverage factor  $k = 2$ , and defines an interval estimated to have a level of confidence of 95 percent

Reference conditions 20 °C, normal incidence solar radiation, horizontal mounting, irradiance level 1000 W/m<sup>2</sup>

#### Measurement process

Metrological characteristic  $S$  in  $[\text{V/(W/m}^2\text{)}]$ : sensitivity to irradiance in the 300 to 3000  $\times 10^{-9} \text{ W/m}^2$  range, with 180° field of view angle, valid for reference conditions  
Calibration method indoor calibration according to ISO 9847, type IIc  
Measurement equipment Hukseflux Solar Radiation Calibration

#### Metrological traceability

Calibration traceability to WRR (World Radiometric Reference)  
Calibration hierarchy from WRR through ISO 9846 and ISO 9847  
Working standard pyranometer type SR30-D1, serial number 2484  
Calibration institute PMOD World Radiation Center, Davos, Switzerland  
Standard sensitivity  $9.94 \times 10^{-6} \text{ V/(W/m}^2\text{)}$

#### Evaluation of the uncertainty of the calibration result

Uncertainty calculation the calibration uncertainty calculated as the square root of the sum of the squares of the calibration uncertainty of the working standard, the uncertainty of the method and the uncertainty due to deviations from the reference conditions is  $\pm 1.0 \%$ .

**Person performing calibration:**  
N.E. Handayani

**Calibration Date:**  
20 SEP, 2019

**Person authorising calibration result of product:**  
M. Rietveld

**Date:**  
24 SEP, 2019



**Hukseflux Thermal Sensors B.V.**  
 www.hukseflux.com  
 info@hukseflux.com

## Product certificate

Pages: 4  
 Release date: 24 SEP, 2019

|                        |   |
|------------------------|---|
| Product code           | <b>SR30-D1</b>  |
| Product identification | <b>serial number 4271</b>                               |
| Product type           | pyranometer   |
| Measurand              | hemispherical solar radiation                           |
| Classification         | secondary standard (ISO 9060), high quality (WMO-No. 8) |

### Calibration result

|                         |   |
|-------------------------|---|
| Sensitivity             | $S = 10.41 \times 10^{-6} \text{ V/(W/m}^2\text{)}$ |
| Calibration uncertainty | $\pm 0.10 \times 10^{-6} \text{ V/(W/m}^2\text{)}$  |

the number following the  $\pm$  symbol is the expanded uncertainty with a coverage factor  $k = 2$ , and defines an interval estimated to have a level of confidence of 95 percent

### Product specifications and conformity

|    |                              |   |
|----|------------------------------|---|
| 1: | ISO 9060 secondary standard  | <b>verified</b>   |
| 2: | resistance                   | <b>19.7 <math>\Omega</math></b>                               |
| 3: | insulation resistance        | <b><math>&gt; 100 \times 10^6 \Omega</math></b>               |
| 4: | response time (95 %)         | <b>3.7 s</b>  |
| 5: | temperature response         | <b>verified</b>   |
| 6: | directional response         | <b>verified</b>   |
| 7: | tilt measurement uncertainty | <b><math>\pm 1^\circ</math> (0 to 90 <math>^\circ</math>)</b> |

**Table 0.1** connections

| PIN | WIRE   |                   |
|-----|--------|-------------------|
| 1   | Brown  | VDC [+]           |
| 4   | Black  | VDC [-]           |
| 3   | Blue   | not connected     |
| 2   | White  | RS-485 B / B' [+] |
| 5   | Grey   | RS-485 A / A' [-] |
|     | Yellow | shield            |

Calibration procedure according to ISO 9847. Traceability of calibration is to the WRR (World Radiometric Reference) maintained at the World Radiation Center in Davos, Switzerland.

Please consult the user manual for set up, operation and maintenance instructions, and information on measurement uncertainty during actual use.

**Person authorising acceptance and release of product:**  
 M. Rietveld

**Date:**  
 24 SEP, 2019



**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

## Directional response

Pages: 4  
Release date: 24 SEP, 2019

|                        |   |
|------------------------|---|
| Product code           | <b>SR30-D1</b>  |
| Product identification | <b>serial number 4271</b>                               |
| Product type           | pyranometer   |
| Measurand              | hemispherical solar radiation                           |
| Classification         | secondary standard (ISO 9060), high quality (WMO-No. 8) |

### Characterisation result

Directional response  $\leq \pm 6.3 \text{ W/m}^2$

### Measurement process

Characterised parameter dependence of sensitivity resulting from the direction of irradiance (a measure of the deviations from an ideal cosine response and its azimuthal variation)

Measurement functions  $C_{rel} = S(\theta)/(S(0) \cdot \cos(\theta) - 1) \cdot 100 \%$   
with  $C_{rel}$  the deviation from an ideal cosine response at zenith angle  $\theta$  in [%],  $S(\theta)$  the sensitivity to beam irradiance at zenith angle  $\theta$  in  $[V/(W/m^2)]$ ,  $S(0)$  the sensitivity to beam irradiance at normal incidence,  $\theta$  the incoming angle from zenith in  $[\circ]$   
 $C_{abs} = (S(\theta)/(S(0) \cdot \cos(\theta) - 1)) \cdot \cos(\theta) \cdot 1000$   
with  $C_{abs}$  the directional response as defined below in  $[W/m^2]$

Measurement equipment Hukseflux Directional Response Characterisation

### Conformity assessment

Definition of measurand The directional response is the error caused by assuming that the reported sensitivity is valid when measuring from any direction a beam whose normal incidence is  $1000 \text{ W/m}^2$

Acceptance interval ISO 9060 specifies a limit on the directional response for a secondary standard pyranometer of  $\pm 10 \text{ W/m}^2$

Conclusion Conformity verified

**Table 0.2** directional response test result

| DIRECTIONAL RESPONSE TEST |                                  |                  |                                  |                  |                                  |                  |                                  |                  |
|---------------------------|----------------------------------|------------------|----------------------------------|------------------|----------------------------------|------------------|----------------------------------|------------------|
| azimuth                   | North                            |                  | East                             |                  | South                            |                  | West                             |                  |
| zenith                    | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] |
| 40 °                      | +0.8                             | +0.1             | -1.0                             | -0.1             | -4.3                             | -0.6             | -5.1                             | -0.7             |
| 60 °                      | +0.2                             | +0.0             | -1.7                             | -0.3             | -5.6                             | -1.1             | -3.4                             | -0.7             |
| 70 °                      | -0.4                             | -0.1             | -2.3                             | -0.7             | -6.3                             | -1.8             | -3.9                             | -1.1             |
| 80 °                      | +2.4                             | +1.4             | +0.3                             | +0.2             | -1.9                             | -1.1             | +0.2                             | +0.1             |

Person performing characterisation:  
K. Ismail

Date:  
19 SEP, 2019





**Hukseflux Thermal Sensors B.V.**  
 www.hukseflux.com  
 info@hukseflux.com

## Temperature response

Pages: 4  
 Release date: 24 SEP, 2019

|                        |   |
|------------------------|---|
| Product code           | <b>SR30-D1</b>  |
| Product identification | <b>serial number 4271</b>                               |
| Product type           | pyranometer   |
| Measurand              | hemispherical solar radiation                           |
| Classification         | secondary standard (ISO 9060), high quality (WMO-No. 8) |

### Characterisation result

|                           |  |
|---------------------------|--|
| Temperature response      | $< \pm 0.06 \% (-30 \text{ to } +50 \text{ }^{\circ}\text{C})$   |
| Temperature coefficients* | $a = -17.9627 \times 10^{-6} \text{ }^{\circ}\text{C}^{-2}$<br>$b = 4.9884 \times 10^{-4} \text{ }^{\circ}\text{C}^{-1}$<br>$c = 0.9972$ |

\* These temperature coefficients are applied internally in the instrument

### Measurement process

|                         |   |
|-------------------------|---|
| Characterised parameter | dependence of sensitivity to ambient temperature  |
| Measurement function    | $S(T) = S_0(a \cdot T^2 + b \cdot T + c)$<br>with $S(T)$ sensitivity in $[\text{V}/(\text{W}/\text{m}^2)]$ at an instrument body temperature $T$ , $S_0$ sensitivity at $20 \text{ }^{\circ}\text{C}$ instrument body temperature, $T$ the instrument body temperature in $[\text{ }^{\circ}\text{C}]$ , $a$ , $b$ and $c$ the temperature coefficients determined from a second order polynomial fit |
| Measurement equipment   | Hukseflux Temperature Response Characterisation   |

### Conformity assessment

|                          |   |
|--------------------------|---|
| Definition of measurand* | Temperature response is the remaining percentage deviation in sensitivity due to change in ambient temperature within a temperature interval after the temperature coefficients are applied |
| Temperature interval     | $-30 \text{ to } +50 \text{ }^{\circ}\text{C}$  |
| Acceptance interval      | Hukseflux specifies a limit on the temperature response for a SR30-D1 of $\pm 0.4 \%$   |
| Conclusion               | Conformity verified   |

\* This is an adaptation of the definition in ISO 9060, which specifies a limit on the temperature response for a secondary standard pyranometer of 2 % within a temperature interval of 50 K.

**Table 0.3 temperature dependence test result**

| TEMPERATURE DEPENDENCE TEST |         |         |         |         |         |
|-----------------------------|---------|---------|---------|---------|---------|
| T [ $^{\circ}\text{C}$ ]    | -30     | -10     | 10      | 30      | 50      |
| remaining deviation         | +0.02 % | -0.04 % | -0.01 % | +0.06 % | -0.03 % |

**Person performing characterisation:**  
 M. Rietveld

**Date:**  
 18 SEP, 2019



**Hukseflux Thermal Sensors B.V.**  
 www.hukseflux.com  
 info@hukseflux.com

## Tilt sensor characterisation

Pages: 4  
 Release date: 24 SEP, 2019

|                        |   |
|------------------------|---|
| Product code           | <b>SR30-D1</b>  |
| Product identification | <b>serial number 4271</b>                               |
| Product type           | pyranometer   |
| Measurand              | hemispherical solar radiation                           |
| Classification         | secondary standard (ISO 9060), high quality (WMO-No. 8) |

| Characterisation result*      | x-axis                    | y-axis                   | z-axis                    |
|-------------------------------|---------------------------|--------------------------|---------------------------|
| gain                          | 1.0100                    | 0.9818                   | 1.0199                    |
| offset                        | -348                      | 315                      | 40                        |
| temperature coefficient $a_0$ | $-0.2698 \times 10^{-12}$ | $0.1461 \times 10^{-12}$ | $-0.0027 \times 10^{-12}$ |
| temperature coefficient $a_1$ | -0.8986                   | 2.3715                   | -1.9106                   |
| temperature coefficient $a_2$ | $0.0527 \times 10^{-2}$   | $-0.4616 \times 10^{-2}$ | $-0.4013 \times 10^{-2}$  |
| temperature coefficient $a_3$ | $-0.6036 \times 10^{-4}$  | $0.0442 \times 10^{-4}$  | $-0.9222 \times 10^{-4}$  |

\* These gains, offsets and temperature coefficients are applied internally in the instrument

### Measurement process

|                              |   |
|------------------------------|---|
| Characterised parameters     | tilt sensor gains and offsets   |
| Measurement equation         | $\theta = 360/2\pi \cdot \arctan((x^2 + y^2)^{1/2}/z)$ $x, y, z = \text{gain}_{x,y,z} \cdot \text{raw}_{x,y,z} + \text{offset}_{x,y,z} + d_{x,y,z}(T)$ $d_{x,y,z}(T) = a_{0x,0y,0z} + a_{1x,1y,1z} \cdot T + a_{2x,2y,2z} \cdot T^2 + a_{3x,3y,3z} \cdot T^3$ <p>with <math>\theta</math> the sensor tilt angle with respect to the horizontal in [°],<br/>           atan the arctangent function, x, y and z the corrected accelerometer counts, <math>\text{gain}_{x,y,z}</math> the tilt sensor gains, <math>\text{raw}_{x,y,z}</math> the raw accelerometer counts, <math>\text{offset}_{x,y,z}</math> the tilt sensor offsets, <math>d_{x,y,z}(T)</math> the correction for temperature dependence of the tilt measurement at an instrument body temperature T, <math>a_0</math>, <math>a_1</math>, <math>a_2</math> and <math>a_3</math> the temperature coefficients determined from a third order polynomial fit. Labels x, y and z refer to the three accelerometer axes.</p> |
| Measurement process          | <p>Alignment with the bubble level is attained in horizontal position by introducing gains and offsets.</p> <p>Gains and offsets are determined in horizontal position and at a tilt angle of 90 °. Temperature dependence of the tilt measurement is determined at a tilt angle of 90 ° between -30 and + 50 °C.</p>   |
| Measurement method           | Hukseflux Tilt Sensor Characterisation  |
| <b>Conformity assessment</b> |   |
| Description of assessment    | The tilt measurement uncertainty is verified in horizontal position and at a tilt angle of 90 °   |
| Acceptance interval          | The tilt measurement uncertainty is specified at $\pm 1^\circ$ (0 to 90 °)  |
| Conclusion                   | Conformity verified   |

**Person performing tilt sensor characterisation:**  
 L. Asaa

**Date:**  
 24 SEP, 2019



**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

## Calibration certificate

Pages 1  
Release date: 24 SEP, 2019

Product code **SR20-T2**  
Product identification **serial number 10546**  
Product type pyranometer  
Measurand hemispherical solar radiation

### Calibration result

Sensitivity  **$S = 15.87 \times 10^{-6} \text{ V/(W/m}^2\text{)}$**   
Calibration uncertainty  **$\pm 0.16 \times 10^{-6} \text{ V/(W/m}^2\text{)}$**

the number following the  $\pm$  symbol is the expanded uncertainty with a coverage factor  $k = 2$ , and defines an interval estimated to have a level of confidence of 95 percent

Reference conditions 20 °C, normal incidence solar radiation, horizontal mounting, irradiance level 1000 W/m<sup>2</sup>

### Measurement process

Metrological characteristic S in [V/(W/m<sup>2</sup>)]: sensitivity to irradiance in the 300 to 3000 x 10<sup>-9</sup> m range, with 180° field of view angle, valid for reference conditions  
Calibration method indoor calibration according to ISO 9847, type IIc  
Measurement equipment Hukseflux Solar Radiation Calibration

### Metrological traceability

Calibration traceability to WRR (World Radiometric Reference)  
Calibration hierarchy from WRR through ISO 9846 and ISO 9847  
Working standard pyranometer type SR20, serial number 5039  
Calibration institute PMOD World Radiation Center, Davos, Switzerland  
Standard sensitivity  $14.60 \times 10^{-6} \text{ V/(W/m}^2\text{)}$

### Evaluation of the uncertainty of the calibration result

Uncertainty calculation the calibration uncertainty calculated as the square root of the sum of the squares of the calibration uncertainty of the working standard, the uncertainty of the method and the uncertainty due to deviations from the reference conditions is  $\pm 1.0 \%$ .

**Person performing calibration:**  
D. Bemelman

**Calibration Date:**  
24 SEP, 2019

**Person authorising calibration result of product:**  
H.E. Brouwer

**Date:**  
24 SEP, 2019





**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

## Product certificate

Pages: 3  
Release date: 24 SEP, 2019

Product code **SR20-T2**  
Product identification **serial number 10546**  
Product type pyranometer  
Measurand hemispherical solar radiation  
Classification secondary standard (ISO 9060), high quality (WMO-No. 8)

### Calibration result

Sensitivity  **$S = 15.87 \times 10^{-6} \text{ V/(W/m}^2\text{)}$**   
Calibration uncertainty  **$\pm 0.16 \times 10^{-6} \text{ V/(W/m}^2\text{)}$**

the number following the  $\pm$  symbol is the expanded uncertainty with a coverage factor  $k = 2$ , and defines an interval estimated to have a level of confidence of 95 percent

Measurement function  **$E = U/S$**   
with E irradiance in  $[\text{W/m}^2]$ , U voltage output in [V]

### Product specifications and conformity

|    |                             |   |
|----|-----------------------------|---|
| 1: | ISO 9060 secondary standard | <b>verified</b>                                 |
| 2: | resistance                  | <b>65.7 <math>\Omega</math></b>                 |
| 3: | insulation resistance       | <b><math>&gt; 100 \times 10^6 \Omega</math></b> |
| 4: | response time (95 %)        | <b>4.0 s</b>                                    |
| 5: | temperature response*       | <b>verified</b>                                 |
| 6: | directional response        | <b>verified</b>                                 |

\*see separate certificate; result may be used to improve measurement quality

**Table 0.1** connections

| PIN | WIRE   |                              |
|-----|--------|------------------------------|
| 2   | Red    | 10 k $\Omega$ thermistor [+] |
| 3   | Pink   | 10 k $\Omega$ thermistor [+] |
| 6   | Blue   | 10 k $\Omega$ thermistor [-] |
| 8   | Grey   | 10 k $\Omega$ thermistor [-] |
| 1   | Brown  | heater                       |
| 4   | Yellow | heater                       |
| 9   | Black  | ground                       |
| 7   | White  | signal [+]                   |
| 5   | Green  | signal [-]                   |

The 10 k $\Omega$  thermistor is a single four-wire thermistor measuring instrument body temperature.

Calibration procedure according to ISO 9847. Traceability of calibration is to the WRR (World Radiometric Reference) maintained at the World Radiation Center in Davos, Switzerland.

Please consult the user manual for set up, operation and maintenance instructions, and information on measurement uncertainty during actual use.

**Person authorising acceptance and release of product:**  
H.E. Brouwer

**Date:**  
24 SEP, 2019



**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

## Directional response

Pages: 3  
Release date: 24 SEP, 2019

Product code **SR20-T2**  
Product identification **serial number 10546**  
Product type pyranometer  
Measurand hemispherical solar radiation  
Classification secondary standard (ISO 9060), high quality (WMO-No. 8)

### Characterisation result

Directional response  $\leq \pm 9.5 \text{ W/m}^2$

### Measurement process

Characterised parameter dependence of sensitivity resulting from the direction of irradiance (a measure of the deviations from an ideal cosine response and its azimuthal variation)

Measurement functions  $C_{rel} = S(\theta)/(S(0) \cdot \cos(\theta) - 1) \cdot 100 \%$   
with  $C_{rel}$  the deviation from an ideal cosine response at zenith angle  $\theta$  in [%],  $S(\theta)$  the sensitivity to beam irradiance at zenith angle  $\theta$  in  $[V/(W/m^2)]$ ,  $S(0)$  the sensitivity to beam irradiance at normal incidence,  $\theta$  the incoming angle from zenith in  $[\circ]$   
 $C_{abs} = (S(\theta)/(S(0) \cdot \cos(\theta) - 1)) \cdot \cos(\theta) \cdot 1000$   
with  $C_{abs}$  the directional response as defined below in  $[W/m^2]$   
Measurement equipment Hukseflux Directional Response Characterisation

### Conformity assessment

Definition of measurand The directional response is the error caused by assuming that the reported sensitivity is valid when measuring from any direction a beam whose normal incidence is  $1000 \text{ W/m}^2$   
Acceptance interval ISO 9060 specifies a limit on the directional response for a secondary standard pyranometer of  $\pm 10 \text{ W/m}^2$   
Conclusion Conformity verified

**Table 0.2** directional response test result

| DIRECTIONAL RESPONSE TEST |                                  |                  |                                  |                  |                                  |                  |                                  |                  |
|---------------------------|----------------------------------|------------------|----------------------------------|------------------|----------------------------------|------------------|----------------------------------|------------------|
| azimuth                   | North                            |                  | East                             |                  | South                            |                  | West                             |                  |
| zenith                    | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] | $C_{abs}$<br>[W/m <sup>2</sup> ] | $C_{rel}$<br>[%] |
| 40 °                      | -1.7                             | -0.2             | -2.0                             | -0.3             | -0.6                             | -0.1             | -4.6                             | -0.6             |
| 60 °                      | -5.1                             | -1.0             | -6.2                             | -1.2             | -5.0                             | -1.0             | -3.6                             | -0.7             |
| 70 °                      | -7.7                             | -2.3             | -9.5                             | -2.8             | -8.0                             | -2.4             | -6.6                             | -1.9             |
| 80 °                      | -7.6                             | -4.4             | -8.5                             | -4.9             | -7.7                             | -4.5             | -6.9                             | -4.0             |

**Person performing characterisation:**  
L. Asaa

**Date:**  
20 SEP, 2019





**Hukseflux Thermal Sensors B.V.**  
www.hukseflux.com  
info@hukseflux.com

## Temperature response

Pages: 3  
Release date: 24 SEP, 2019

Product code **SR20-T2**  
Product identification **serial number 10546**  
Product type pyranometer  
Measurand hemispherical solar radiation  
Classification secondary standard (ISO 9060), high quality (WMO-No. 8)

### Characterisation result

Temperature response  $\pm 0.2 \%$   
Temperature coefficients  
 $a = -7.2194 \times 10^{-6} \text{ }^{\circ}\text{C}^{-2}$   
 $b = 2.2014 \times 10^{-4} \text{ }^{\circ}\text{C}^{-1}$   
 $c = 0.9985$

### Measurement process

Characterised parameter dependence of sensitivity to ambient temperature  
Measurement function  $S(T) = S_0 \cdot (a \cdot T^2 + b \cdot T + c)$   
with  $S(T)$  sensitivity in  $[\text{V}/(\text{W}/\text{m}^2)]$  at an instrument body temperature  $T$ ,  $S_0$  sensitivity at  $20 \text{ }^{\circ}\text{C}$  instrument body temperature,  $T$  the instrument body temperature in  $[\text{ }^{\circ}\text{C}]$ ,  $a$ ,  $b$  and  $c$  the temperature coefficients determined from a second order polynomial fit

Measurement equipment Hukseflux Temperature Response Characterisation

### Conformity assessment

Definition of measurand Temperature response is the percentage deviation in sensitivity due to change in ambient temperature within an interval of 50 K  
Temperature interval -10 to  $+40 \text{ }^{\circ}\text{C}$   
Acceptance interval ISO 9060 specifies a limit on the temperature response for a secondary standard pyranometer of 2 %  
Conclusion Conformity verified

**Table 0.3** temperature dependence test result

#### TEMPERATURE DEPENDENCE TEST

| T [ $^{\circ}\text{C}$ ] | -30    | -20    | -10    | 0      | 10     | 20     | 30     | 40     | 50     |
|--------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|
| $\frac{S(T) - S_0}{S_0}$ | -1.5 % | -0.9 % | -0.4 % | -0.2 % | +0.0 % | +0.0 % | -0.1 % | -0.4 % | -0.9 % |

**Person performing characterisation:**

H.A. Kanij

**Date:**

19 SEP, 2019






Delta-T Devices Ltd

**SPN1 Sunshine Pyranometer**

# Calibration Certificate

This is to certify that the Sunshine Pyranometer type SPN1 identified below has been calibrated in accordance with Delta-T Devices Ltd standard production procedures and conforms to the specifications as detailed.

|                      |  |
|----------------------|--|
| Serial Number        | SPN1 – A2057   |
| Date                 | 24/09/19   |
| Authorised Signature |  |

We recommend that this instrument is recalibrated every 2 years.

**Traceability**

The SPN1 is calibrated under a uniform light source which simulates the solar spectrum, against a transfer standard SPN1. The transfer standard is calibrated outdoors against a Kipp & Zonen CM21 secondary standard pyranometer (calibration traceable to the World Radiometric Reference), with solar tracker and shading disk for diffuse measurement.

**Accuracy, Total (Global) and Diffuse radiation**

When correctly calibrated, the expected accuracy is given in the table below. The figures give 95% confidence limits, i.e. 95% of individual readings will be within the stated limits under normal climatic conditions.

|                             |   |
|-----------------------------|---|
| Overall accuracy:           | $\pm 5\%$ daily integrals<br>$\pm 5\% \pm 10 \text{ W.m}^{-2}$ hourly averages<br>$\pm 8\% \pm 10 \text{ W.m}^{-2}$ individual readings |
| Range                       | 0 to $>2000 \text{ W.m}^{-2}$   |
| Analogue output sensitivity | $1\text{mV} = 1 \text{ W.m}^{-2}$   |

**Delta-T Devices Ltd**

130 Low Road, Burwell, Cambridge, CB25 0EJ, UK

Tel: +44 1638 742922 Fax: +44 1638 743155

email: [sales@delta-t.co.uk](mailto:sales@delta-t.co.uk) web: [www.delta-t.co.uk](http://www.delta-t.co.uk)

Calibration Certificate Silicon Irradiance Sensor

Sensor Type: SI-mV-85-A  
Serial No.: 85-00205-17-19350068  
Comment:

**Irradiance Calibration with Artificial Light in Comparison to a Reference Cell**

Calibrated by: Huhnstock-Breuer  
Date / Time: 28.08.2019 13:41

|                | Type              | Calibration<br>$\mu\text{V/W/m}^2$ | Temperature Coefficient<br>$1/^\circ\text{C}$ | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Irradiance <sup>1)</sup><br>$\text{W/m}^2$ |
|----------------|-------------------|------------------------------------|---|--------------|---------------------------------|--|
| Reference Cell | Si-Ref mono PTB-1 | 56,51                              | 0,00067                                       | 56,953       | 30,76                           | 1004,0                                     |
|                | Type              | Irradiance<br>$\text{W/m}^2$       | Correction Factor <sup>2)</sup>               | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Calibration<br>$\mu\text{V/W/m}^2$         |
| Test Object    | SI-mV-85-A        | 1004,0                             | 0,995006                                      | 58,777       | 32,17                           | 58,25                                      |

**Test Equipment Irradiance Calibration**

| Manufacturer                          | Type              | Serial No.           | Calibration Certificate   | Trace |
|---------------------------------------|-------------------|----------------------|---------------------------|-------|
| Ingenieurbüro Mencke & Tegtmeyer GmbH | Si-Ref mono PTB-1 | 02-20002-05-15309999 | 47109-PTB-18              | PTB   |
| Gantner Instruments                   | IDL100            | 191667               | 098220-02 D-K-15019-01-00 | DKD   |
|                                       | ISM111            | 078743               | 098221-02 D-K-15019-01-00 | DKD   |
| OMEGA Engineering                     | INS10             | 9894                 | J.                        | J.    |

$$^{1)} \text{Irradiance} = \frac{\text{Output} \cdot 1000}{\text{Calibration} \cdot (1 + \text{Temperature Coefficient} \cdot (\text{Temperature} - 25))}$$

$$^{2)} \text{Calibration} = \frac{\text{Output} \cdot 1000 \cdot \text{Correction Factor}}{\text{Irradiance}}$$

<sup>3)</sup> Individual calculated for each Calibration Process, must not be used for Outdoor Application.

Calibration Certificate Silicon Irradiance Sensor

Sensor Type: SI-mV-85-A  
Serial No.: 85-00205-17-19350069  
Comment:

## Irradiance Calibration with Artificial Light in Comparison to a Reference Cell

Calibrated by: Huhnstock-Breuer  
Date / Time: 28.08.2019 13:41

|                | Type              | Calibration<br>$\mu\text{V/W/m}^2$ | Temperature Coefficient<br>$1/^\circ\text{C}$ | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Irradiance <sup>1)</sup><br>$\text{W/m}^2$ |
|----------------|-------------------|------------------------------------|---|--------------|---------------------------------|--|
| Reference Cell | Si-Ref mono PTB-1 | 56,51                              | 0,00067                                       | 56,953       | 30,76                           | 1004,0                                     |
|                | Type              | Irradiance<br>$\text{W/m}^2$       | Correction Factor <sup>2)</sup>               | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Calibration<br>$\mu\text{V/W/m}^2$         |
| Test Object    | SI-mV-85-A        | 1004,0                             | 0,995519                                      | 58,112       | 31,43                           | 57,62                                      |

## Test Equipment Irradiance Calibration

| Manufacturer                          | Type              | Serial No.           | Calibration Certificate   | Trace |
|---------------------------------------|-------------------|----------------------|---------------------------|-------|
| Ingenieurbüro Mencke & Tegtmeyer GmbH | Si-Ref mono PTB-1 | 02-20002-05-15309999 | 47109-PTB-18              | PTB   |
| Gantner Instruments                   | IDL100            | 191667               | 098220-02 D-K-15019-01-00 | DKD   |
|                                       | ISM111            | 078743               | 098221-02 D-K-15019-01-00 | DKD   |
| OMEGA Engineering                     | INS10             | 9894                 | J.                        | J.    |

$$^{1)} \text{Irradiance} = \frac{\text{Output} \cdot 1000}{\text{Calibration} \cdot (1 + \text{Temperature Coefficient} \cdot (\text{Temperature} - 25))}$$

$$^{2)} \text{Calibration} = \frac{\text{Output} \cdot 1000 \cdot \text{Correction Factor}}{\text{Irradiance}}$$

<sup>3)</sup> Individual calculated for each Calibration Process, must not be used for Outdoor Application.





**INGENIEURBÜRO**  
Mencke & Tegtmeier GmbH  
Meßgeräte für die Solartechnik

Schwarzer Weg 43A  
31789 Hameln, Germany  
www.ib-mut.de

#### Calibration Certificate Silicon Irradiance Sensor

Sensor Type: Si-mV-85-A  
Serial No.: 85-00205-17-19350076  
Comment:

#### Irradiance Calibration with Artificial Light in Comparison to a Reference Cell

Calibrated by: Huhnstock-Breuer  
Date / Time: 28.08.2019 13:44

|                | Type              | Calibration<br>$\mu\text{V}/\text{W}/\text{m}^2$ | Temperature Coefficient<br>$1/^\circ\text{C}$ | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Irradiance <sup>1)</sup><br>$\text{W}/\text{m}^2$ |
|----------------|-------------------|--|---|--------------|---------------------------------|---|
| Reference Cell | Si-Ref mono PTB-1 | 56,51  | 0,00067                                       | 56,953       | 30,76                           | 1004,0  |
|                | Type              | Irradiance<br>$\text{W}/\text{m}^2$              | Correction Factor <sup>3)</sup>               | Output<br>mV | Temperature<br>$^\circ\text{C}$ | Calibration<br>$\mu\text{V}/\text{W}/\text{m}^2$  |
| Test Object    | Si-mV-85-A        | 1004,0   | 0,995901                                      | 58,396       | 30,88                           | 57,93   |

#### Test Equipment Irradiance Calibration

| Manufacturer                          | Type              | Serial No.           | Calibration Certificate   | Trace |
|---------------------------------------|-------------------|----------------------|---------------------------|-------|
| Ingenieurbüro Mencke & Tegtmeier GmbH | Si-Ref mono PTB-1 | 02-20002-05-15309999 | 47109-PTB-18              | PTB   |
| Gantner Instruments                   | IDL100            | 191667               | 098220-02 D-K-15019-01-00 | DKD   |
|                                       | ISM111            | 078743               | 098221-02 D-K-15019-01-00 | DKD   |
| OMEGA Engineering                     | IN510             | 9894                 | ./. .                     | ./. . |

$$^1) \text{Irradiance} = \frac{\text{Output} \cdot 1000}{\text{Calibration} \cdot (1 + \text{Temperature Coefficient} \cdot (\text{Temperature} - 25))}$$

$$^2) \text{Calibration} = \frac{\text{Output} \cdot 1000 \cdot \text{Correction Factor}}{\text{Irradiance}}$$

<sup>3)</sup> Individual calculated for each Calibration Process, must not be used for Outdoor Application.



1 (1)  
Certificate report no. H47-19330044

## CALIBRATION CERTIFICATE

Instrument PTB110 Barometer  
Serial number R3331024  
Manufacturer Vaisala Oyj, Finland  
Calibration date 14th August 2019

This instrument has been calibrated against a Vaisala PTB220 factory working standard. The Vaisala PTB220 is traceable to the National Institute of Standards and Technology (NIST, USA) via Vaisala Measurement Standards Laboratory (MSL). Vaisala MSL has been accredited by FINAS according to ISO/IEC 17025 standard.

At the time of shipment, the instrument described above was within its operating specifications.

### Calibration results

| Reference pressure<br>hPa | Calculated pressure<br>hPa | Observed voltage<br>Vdc | Correction*<br>hPa | Uncertainty**<br>hPa |
|---------------------------|----------------------------|-------------------------|--------------------|----------------------|
| 510.3                     | 510.2                      | 0.043                   | 0.1                | ± 0.15               |
| 610.0                     | 610.1                      | 0.458                   | -0.1               | ± 0.15               |
| 700.0                     | 700.0                      | 0.833                   | 0.0                | ± 0.15               |
| 809.8                     | 809.8                      | 1.291                   | 0.0                | ± 0.15               |
| 900.0                     | 900.0                      | 1.666                   | 0.0                | ± 0.15               |
| 999.9                     | 999.9                      | 2.083                   | 0.0                | ± 0.15               |
| 1060.1                    | 1060.1                     | 2.334                   | 0.0                | ± 0.15               |
| 1099.9                    | 1099.9                     | 2.500                   | 0.0                | ± 0.15               |

\*To obtain the true pressure, add the correction to the barometer reading. Interpolated corrections may be used at intermediate readings of the scale of the barometer.

\*\*The calibration uncertainty given at 95 % confidence level, k = 2

### Equipment used in calibration

|          |               |                  |                    |
|----------|---------------|------------------|--------------------|
| Type     | Serial number | Calibration date | Certificate number |
| HP34970A | 17403         | 2019-08-12       | 1250-307103583     |
| PTB220   | PA 14018      | 2019-03-21       | K008-C00955        |

### Ambient conditions

Humidity: 37 ± 5 %RH

Temperature: 22 ± 2 °C

Pressure: 1004 ± 20 hPa

  
Technician

This report shall not be reproduced except in full, without the written approval of Vaisala.

Doc214685-B



Vaisala Oyj | PO Box 26, FI-00421 Helsinki, Finland  
Phone +358 9 894 91 | Fax +358 9 8949 2227  
Email firstname.lastname@vaisala.com | www.vaisala.com  
Domicile Vantaa, Finland | VAT FI01244162 | Business ID 0124416-2

## Calibration Certification

**Name and address of the manufacturer:** Sensirion AG  
Laubisruetistrasse 50  
CH-8712 Switzerland

**Description:** Digital Humidity- and Temperature Sensors

- |         |         |
|---------|---------|
| • SHT1x | • SHT2x |
| • SHT3x | • SHT7x |
| • SHTC1 | • SHTW1 |
| • STS21 | • STSC1 |

The above mentioned products are calibrated to meet the specifications according to the corresponding Sensirion data sheet. Each device is individually tested after its calibration.

Sensirion uses transfer standards for the calibration. These transfer standards are themselves subject to a scheduled calibration procedure. The calibration of the reference itself used for the calibration of the transfer standards is performed by an ISO/IEC 17025 accredited laboratory.

The accreditation body is full member of the International Laboratory Accreditation Cooperation ([www.ilac.org](http://www.ilac.org)). Calibration certificates issued by facilities accredited by a signatory to the ILAC Mutual Recognition Arrangement (MRA) are accepted by all signatories to the ILAC MRA.

This provides traceability of measurement to recognized national standards and to units of measurement realized at the "National Physical Laboratory" (NPL) or other recognized national standards laboratories like "Physikalisch-Technische Bundesanstalt" (PTB) or "National Institute of Standards and Technology" (NIST).

Staeafa, November 2015



Stephan Weber,  
Director,  
Head of Quality Management, Sensirion AG



Volker Born  
Manager,  
Head of Quality Engineering, SensirionAG





## CERTIFICATE OF CALIBRATION AND TESTING

|                       |                                       |
|-----------------------|---------------------------------------|
| <b>SERIAL NUMBER:</b> | <b>WS00016673</b>                     |
| <b>CUSTOMER:</b>      | INTELTRONICS INSTRUMENT               |
| <b>P.O. NUMBER:</b>   | 2293 4 DEC 18                         |
| <b>INV NUMBER:</b>    | 149890                                |
| <b>MODEL:</b>         | 03002 WIND SENTRY ANEM & VANE W/J-BOX |

We hereby certify that the sensor serial number specified above has been inspected, tested, and found to comply with all process and material specifications established for the purpose of quality assurance of R . M. Young Company products. Engineering drawings, procedures, and specifications are maintained on file at our premises.

Standards established by R. M. Young Company for calibrating the measuring and test equipment used in controlling product quality are traceable to the National Institute of Standards and Technology (NIST).

Date of Certification: 25 Jan 2019

R. M. Young Company

Ed Chemosky  
Quality Assurance

**R. M. YOUNG COMPANY** 2801 Aero Park Drive, Traverse City Michigan 49686-9171 USA  
TEL: (231) 946-3980 FAX: (231) 946-4772 Email: met.sales@youngusa.com

Model 525 Series Certification/Calibration Information

(form PR-TRL-AL-02.docx)

The sensors go through the certified calibration process to document for record with +/- 1% accuracy.

The recorded error readings for this sensor was: .57 .55

Calibration Date: 7-24-19 S/N: 81181-819

BY: VR

**NOTICE!!!**

During Shipment the tipping assembly has been secured to avoid possible damage to the pivot assembly. Lift off collection and remove rubber band from inside to release tipping mechanism before installation.